




1

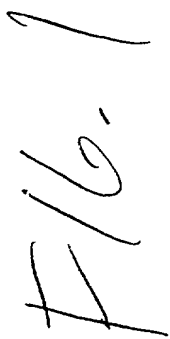

F/6.2

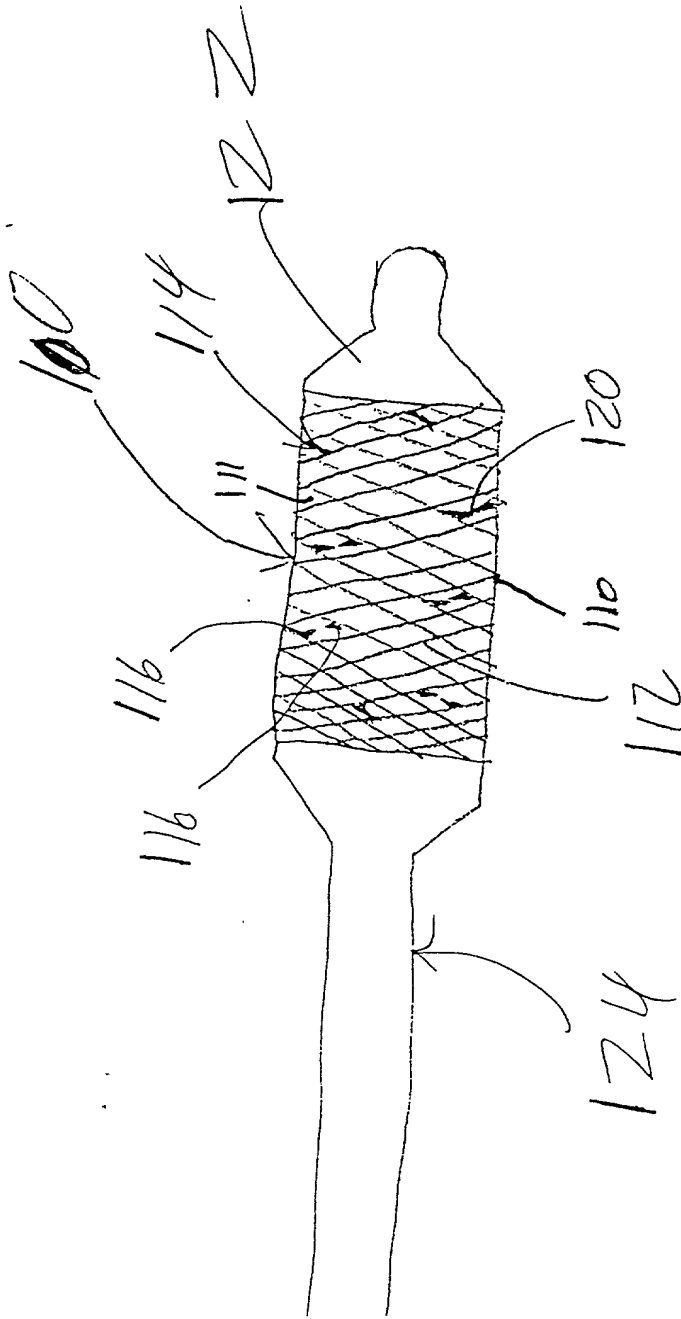


F16.3

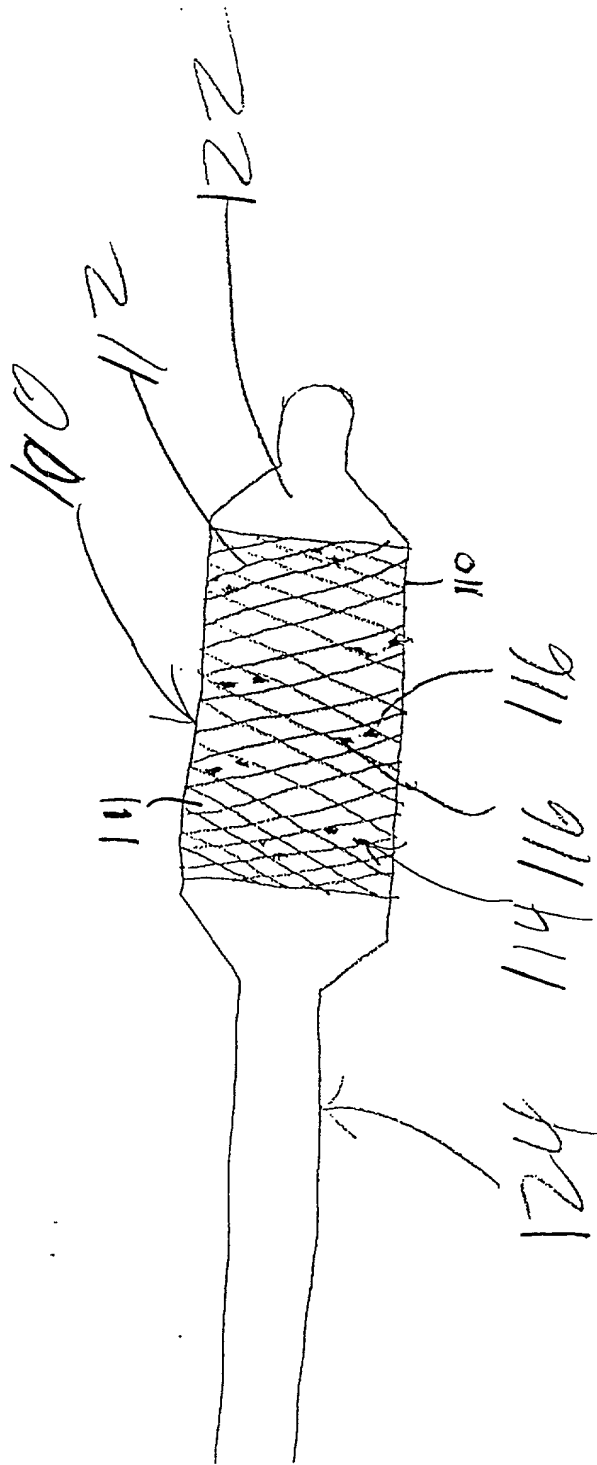

41 v-

094433 033101

094433 033101

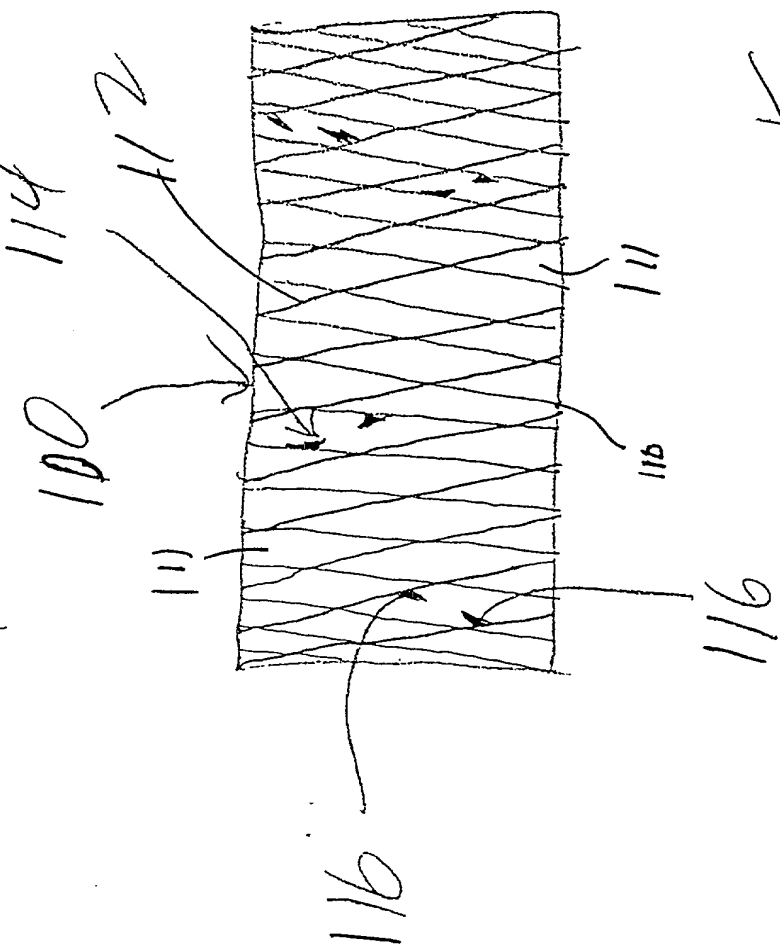

F = 16.4

4/10/00

TOP SECRET

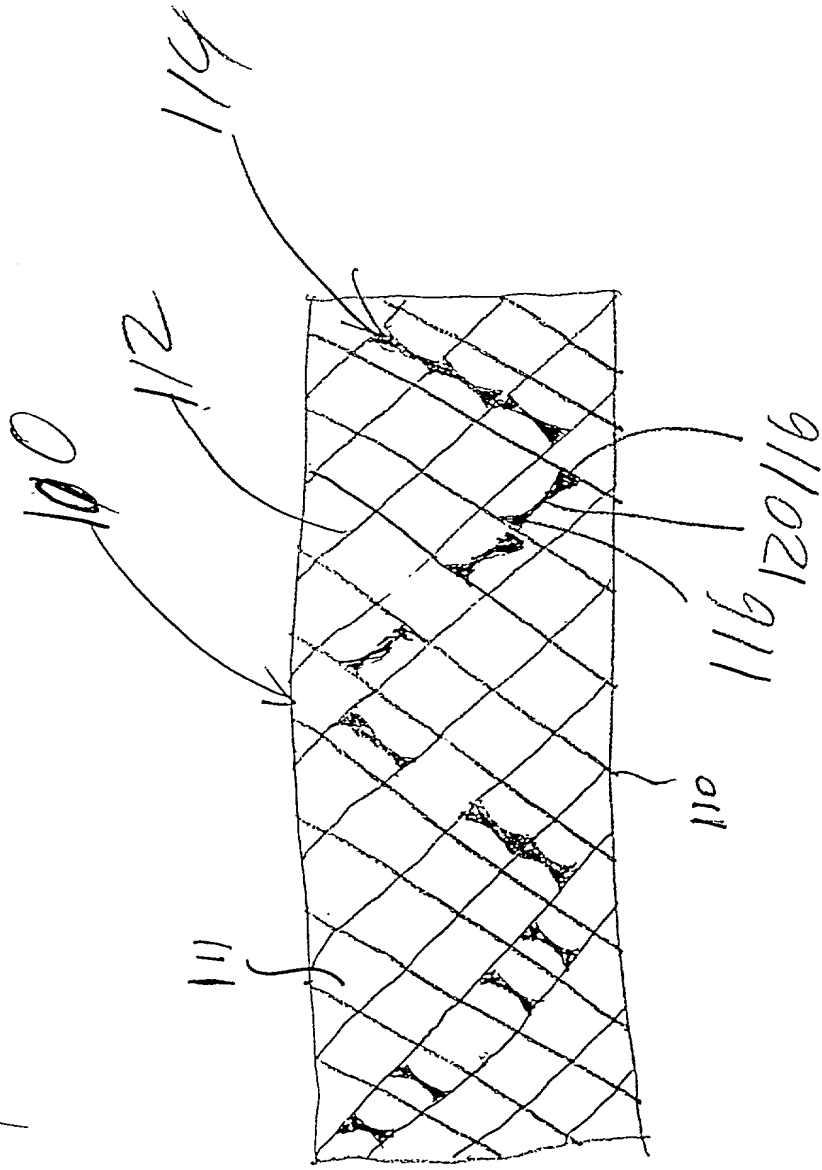


Fig. 5

+10-

09544668.083.001

130

021



F/6.6

2 / 3

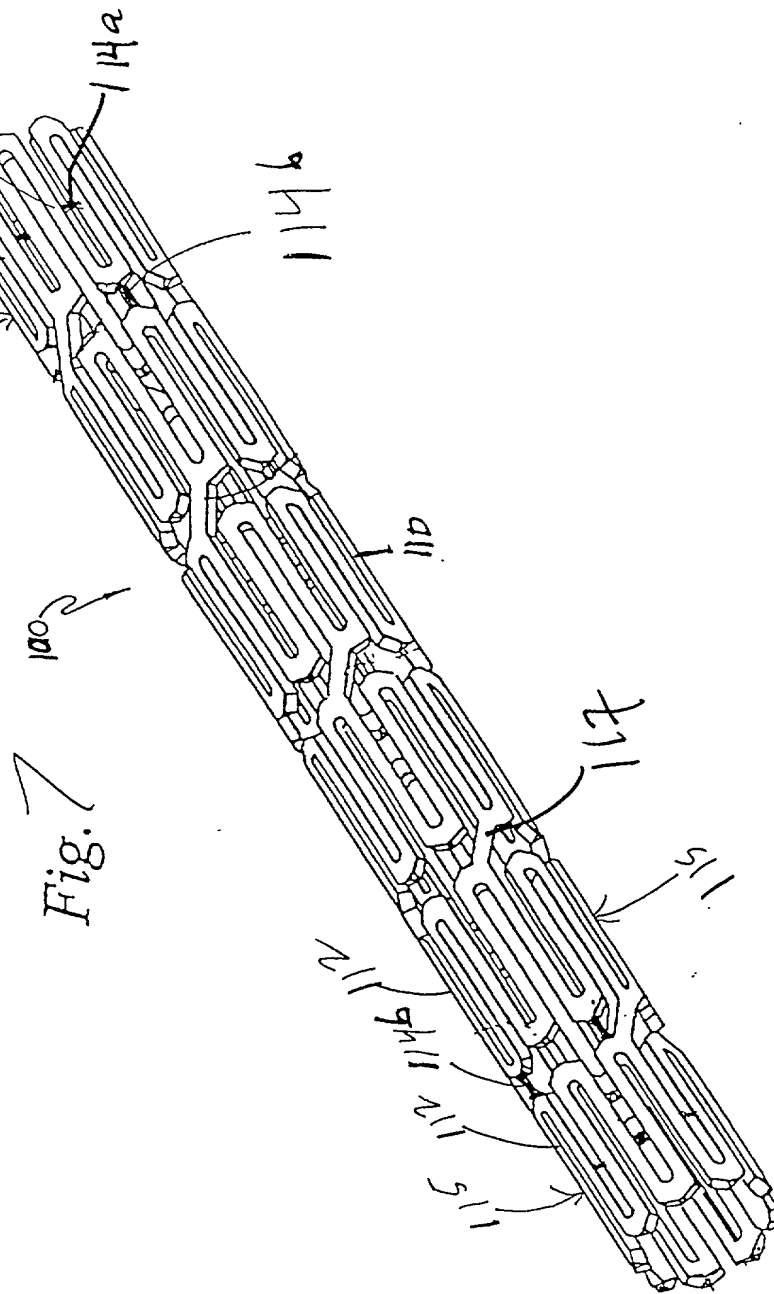


FIG. 3

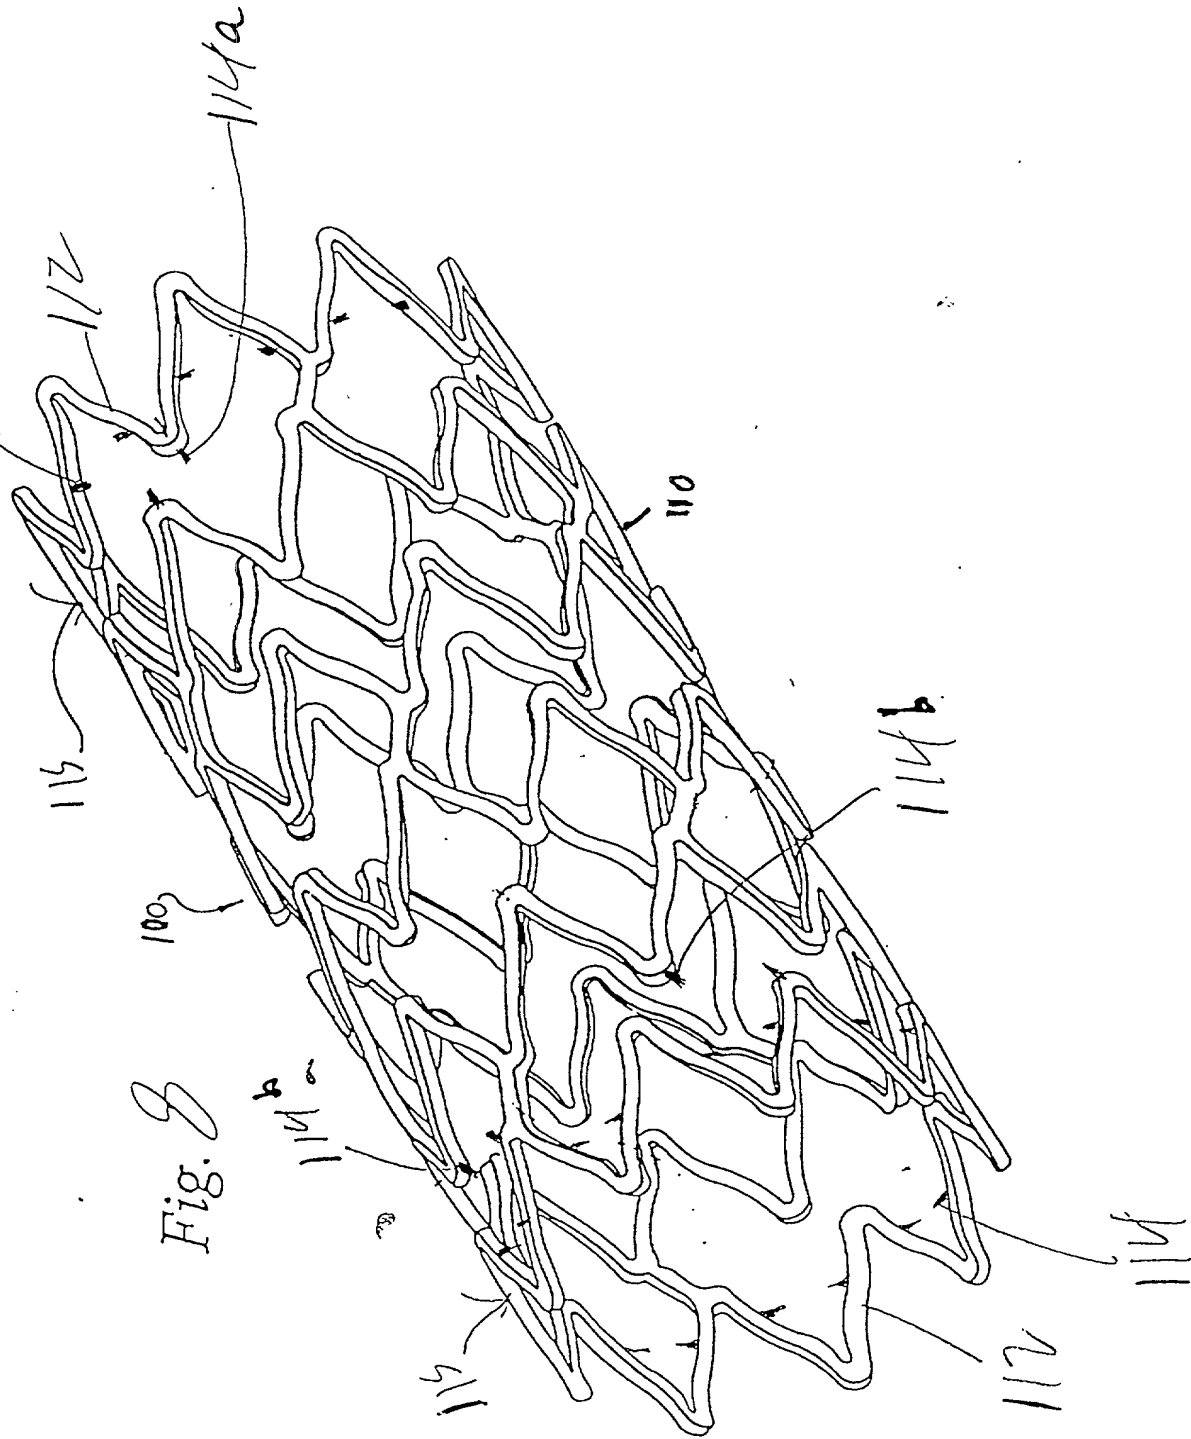




Fig. 9

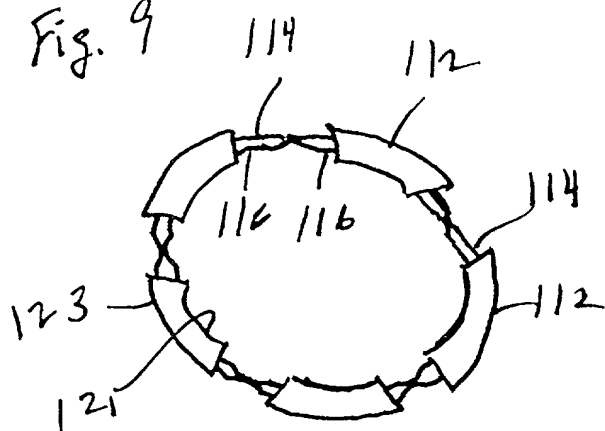


Fig. 10


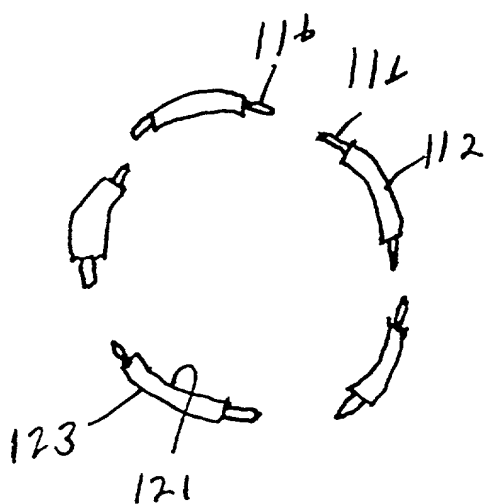


Fig. 11

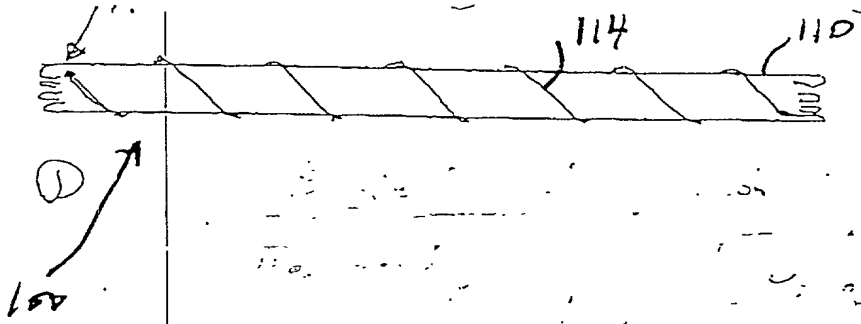

0944560-0301

The stent is tread to continue expanding until

STEP C

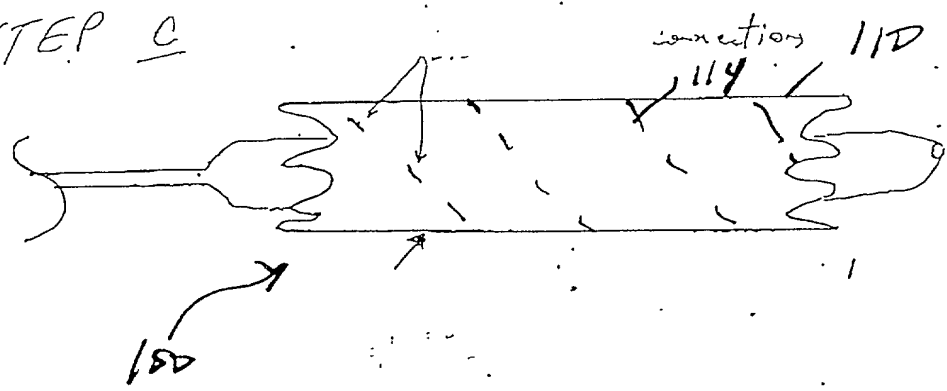


Fig. 12

0344563.003

Fig. 3

